




## 13. Using Enabled Objects to make Combined Volume Measurements for Multiple Objects

- Check the Combine Enabled Objects checkbox. **1**
- Name the combined result or leave with the default name Combined. **2**
- Click Sample Enabled Objects. **3**
- The combined measurements will be reported in the stats review area **4** and added to the log file. **5**

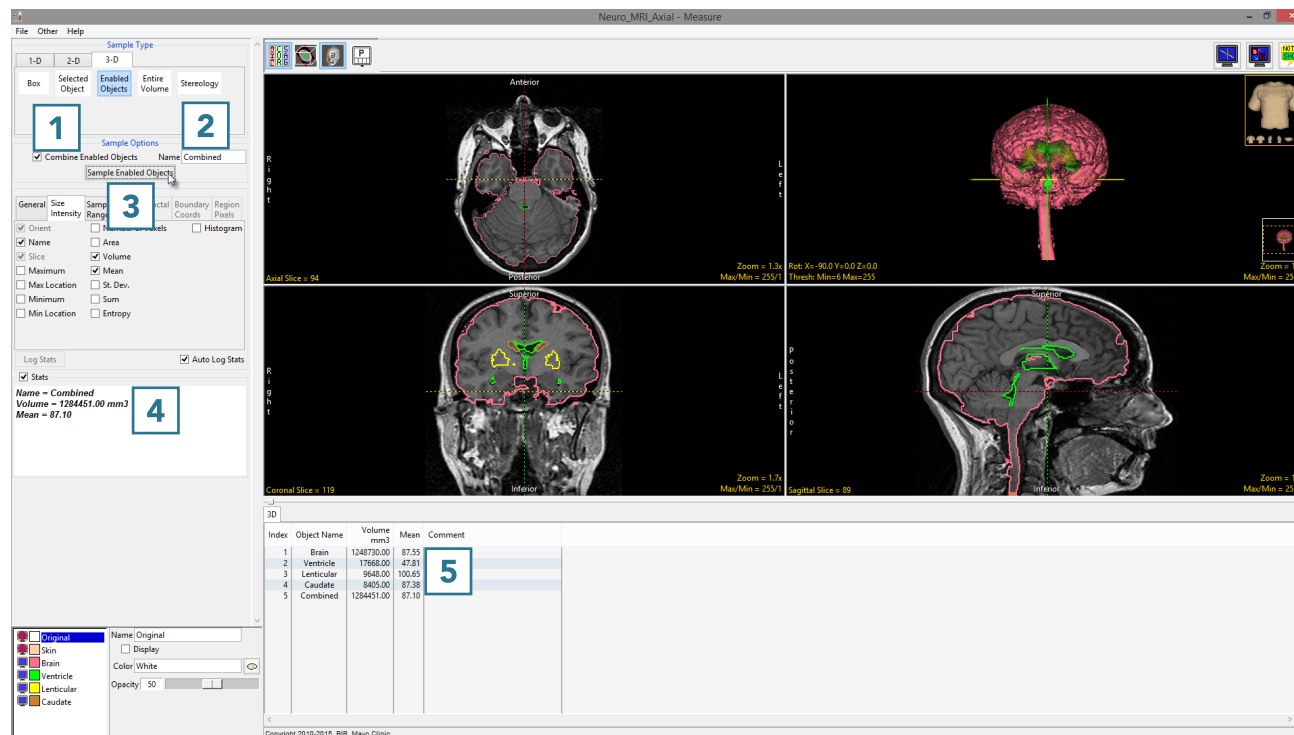

- Checking additional measurement options **17** will automatically update in the Stats review area with the selected measurement for the combined object. **18**
- The measurements for the individual and combined objects will automatically update in the log. **19**

